



# GroStar<sup>®</sup>

AI101G

**GS1 Premium pH Pen**

(Gen II)

## User Guide

Scan to watch the video tutorial



# Contents

	page
<b>01</b> Main Features	2
<b>02</b> Preparation Before First Use	3
<b>03</b> pH Calibration	4
<b>04</b> pH Measurement	5
<b>05</b> Other Functions	5
<b>5.1</b> Reading Hold	5
<b>5.2</b> Temperature Unit Switch	5
<b>5.3</b> Auto. Power Off	5
<b>5.4</b> TruRead Measurement Mode	5
<b>5.5</b> ORP Measurement	5
<b>06</b> Probe Cleaning	6
<b>07</b> Probe Storage	6
<b>08</b> Battery Replacement	7
<b>09</b> Probe Replacement	7
<b>10</b> Notes	8
<b>11</b> Troubleshooting Guide	9
<b>12</b> Technical Specs	10
<b>13</b> Accessories	10
<b>14</b> Limited Warranty	

Thank you for choosing GroStar® GS1 Premium pH Pen Tester (Gen II). This premium pen has been designed specifically for the horticultural market. Since 1991, Apera Instruments has been dedicated to providing advanced lab-grade instruments and sensors. GroStar's intelligent design reduces the guesswork so you can easily manage your crops success.

## 01 Main Features

- Premium pH probe with double-junction, sensor shield and blue gel electrolyte for high accuracy and durability.
- Easy to use design and quick 2-point automatic calibration with electrode condition display.
- 3-Color backlit LCD screen gives you clear readings in different modes even in dark environment.
- Durable structure, IP67 waterproof rating, powered by AAA batteries.
- The pH probe is replaceable, so you don't have to discard the entire pen when the probe reaches its end of life.

**3-Color LCD Screen**


- White for measurement mode
- Green for calibration mode
- Red for calibration error

stands for stabilized reading

L/M/H stands for successful calibration: L is pH 4, M is pH 7, H is pH 10. The icon(s) will disappear after 30 days to remind you for re-calibration.

**Probe Cap**

- Water droplets are added during production to maintain the moisture of the probe. This is normal practice and should not be attributed to used product.
- The fill line shows the level to which you should pour the soaking solution or sample solution.
- For details of probe storage, see Section 7.



	Short Press	Long Press
	1. Power on 2. Manual hold Press again to cancel hold.	Power off
	In measurement mode, press to enter TruRead mode	Start calibration
	In measurement mode, press to switch to mV mode (for ORP test)	Switch between °F and °C

**Sensor Shield**


Protects the sensitive pH glass membrane from accidental damage. Remove it when cleaning the pH sensor.

**Premium pH Probe**


- The Double-junction blue pH sensor significantly improves durability and ease of use.
- The probe is replaceable, saving money in the long run.

## 02 Preparation Before First Use

2.1 Pull out the battery insulation slip, and take off the probe cap.




2.2 Rinse off the probe in clean water, then shake off excess water.

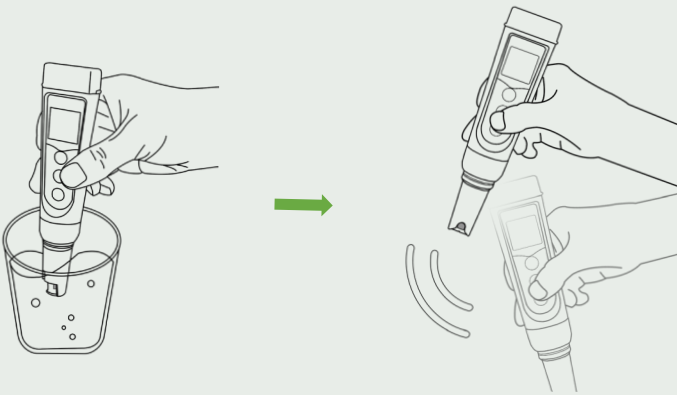

2.3 Perform a 2-point calibration at pH 7 and pH 4. For calibration tutorial, refer to Section 3.

2.4 If you find the probe cap is dried out, soak the probe in 3M KCL soaking solution for 5 minutes before use.

2.5 If the tester hasn't been used for a long time (over 1 month), please soak the probe in the 3M KCL soaking solution for at least 1 hour, then calibrate it before testing.




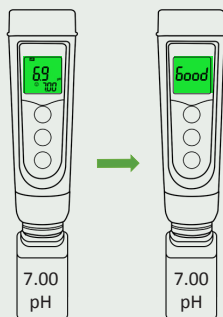
## 03 pH Calibration

- 3.1 Power on the pen and remove the probe cap.




**Always calibrate 7.00 pH first.**



- 3.2 Rinse the probe with clean water and shake-dry, then submerge it in the 7.00 pH standard buffer; **shake the probe vertically in the solution bottle for a few seconds**, then let it stand.


- 3.3 Hold  until screen turns green. The tester starts the automatic calibration. Wait for "Good" to show up (in 10-15 seconds), indicating the calibration is completed, then the tester returns to measurement mode.






Short press any key while calibrating (in green screen) to cancel calibration and return to measurement.

- 3.4  icon will show up on the lower left corner of the screen indicating the tester is successfully calibrated. Repeat Steps 3.2 to 3.3 to calibrate pH 4 using 4.00 pH buffer, then  will show up next to .


You can continue to calibrate pH 10 by repeating Steps 3.2 to 3.3 using 10.01 pH buffer (sold separately), then  will show up to the right of .



Calibrating pH 10 is usually not necessary unless your estimated target pH is greater than 8.0 pH.

- 3.5    will disappear in 30 days after calibration, reminding you to re-calibrate the tester. We recommend calibrating pH at least once a month to ensure accuracy. If you feel like the accuracy might be off, simply test the standard buffers (make sure the buffers are fresh and clean). If a discrepancy is found, then it's time to calibrate again.

- 3.6 After finishing the 2nd point calibration, the slope data of the pH electrode will show up, indicating the health condition of your pH electrode. The closer the slope is to 100%, the better the electrode's condition is. In general, we would consider 97% to 100% as great condition, 93% to 96% as good condition. If below 90%, it means your pH electrode is close to its end of life, and we recommend replacing it to ensure the optimal measurement accuracy.



- 3.7 If the calibration fails, the screen will turn red. For details, see Section 11 Troubleshooting Guide.




Always perform at least a 2-point pH calibration to ensure accuracy. Start with pH 7, followed by pH 4 immediately. If you happened to turn off the pen before calibrating pH 4, you need to start with pH 7 again after rebooting the pen, then pH 4.



## 04 pH Measurement

- 4.1 Power on and remove the probe cap.
- 4.2 Rinse the probe with clean water and shake off excess water.
- 4.3 Fully submerge the probe into the solution at least 1 inch deep, make a quick stir in the solution to remove air bubbles around the probe.
- 4.4 Hold the pen and wait for the reading to stabilize (☺ stays on screen), then record the reading.
- 4.5 Thoroughly rinse off the probe with clean water, then close the probe cap.

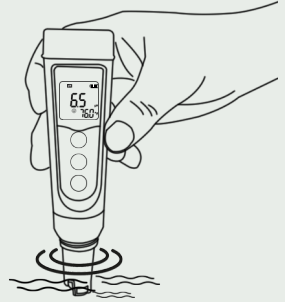

## 05 Other Functions

- 5.1 If necessary, you can manually hold (lock) the reading by short pressing . Press it again to cancel the hold.
- 5.2 Long press to switch temp. unit between °F and °C.
- 5.3 The tester will automatically power off if there is no operation within 10 minutes. If you want to turn off the Auto. Power Off function, power off the tester, and then hold for 5 seconds until you see Auto off. Then it will power on and go to measurement mode automatically.
- 5.4 Short press to enter **TruRead** mode. As you are testing, the pen will automatically record pH measurements after the reading is stabilized for 7 seconds ("01" will show up at the bottom right to indicate the 1st set of data is recorded). After you finish all the test, short press again to check the average, maximum, and minimum values of all the recorded measurements. Then short press again to end TruRead mode and return to normal measurement mode.
- 5.5 The pen can measure ORP with the installation of an ORP probe (SKU: GS5-E, refer to Section 9 on how to replace a probe). The meter will automatically recognize the ORP probe and switch to mV mode. Then you are ready to test the ORP level of your solution.



5.5 The pen can measure ORP with the installation of an ORP probe (SKU: GS5-E, refer to Section 9 on how to replace a probe). The meter will automatically recognize the ORP probe and switch to mV mode. Then you are ready to test the ORP level of your solution.




ORP (Oxidation Reduction Potential) describes the ability of water to break down waste and contaminants. Hydroponic ORP management gives growers the ability to observe and maintain a relative measure of the health of nutrient solutions. The optimal ORP range for your nutrient solutions is 250 – 400 mV.

## 06 Probe Cleaning


- 6.1 The tester is only as accurate as the probe is clean. Always thoroughly rinse off the probe before and after each measurement with pure water or with a wash bottle (tap water is ok. Ideally use RO or distilled water).
- 6.2 For tough contaminants, remove the sensor shield, soak the probe in Apera's cleaning solution or detergent water for 30 minutes. Then use a soft brush to remove the contaminants. Afterwards, soak the probe in 3M KCL soaking solution for at least 1 hour. Rinse it off, then re-calibrate the tester before using again. These cleaning tools can be found in the Probe Care Kit (see Section 13).

## 07 Probe Storage

- 7.1 Under regular usage (daily or weekly use), just make sure the probe cap is wet (with a few water droplets inside), and tightly close the cap with the red O-ring.




- 7.2 For long-term storage (you are not going to use the product for a while), add 3M KCL soaking solution to the Fill line in the probe cap and store the probe in it. Close on the probe cap tightly with the red O-ring.



If you find white crystals around the probe, it is perfectly normal. It is the probe's 3M KCL inner electrolyte that crystalizes over time by its nature. Just rinse them off and use the pen as normal. This chemical is not poisonous nor dangerous, and the probe's performance will not be affected at all.

## 08 Battery Replacement

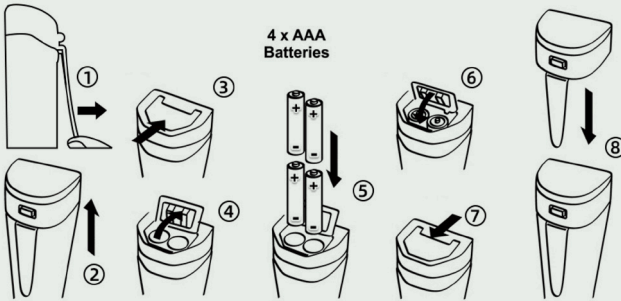


- ① Loosen the battery cap lock.
- ② Pull off the battery cap.
- ③ Slide the battery cover along the OPEN arrow to open the cover.
- ④ Open the battery cover.
- ⑤ Insert the batteries (**ALL POSITIVE SIDES FACING UP**).
- ⑥ Press down the battery cover and hold it.
- ⑦ Slide the battery cover along the LOCK arrow to lock the cover.
- ⑧ Close the battery cap. Make sure to push it all the way down.

The tester's waterproof rating may be compromised if the battery cap is not tightly closed.

## 09

## Probe Replacement



Twist off the probe ring, unplug the old probe; plug in the new probe (make sure to align the connector's position properly), then twist on the probe ring.



pH probes don't last forever. Every pH probe will eventually age and fail even if you don't use it that often. The typical service life of GroStar pH probes is 18-24 months depending on the frequency of usage and how well you keep it clean and properly stored.

We recommend replacing your probe at least every 18 months to ensure the best accuracy.

The nice thing about GroStar pens is that you can just buy a replacement probe instead of a whole new tester.

## 10


## Notes

- 10.1 Never store the probe in pure water such as tap water, RO water, distilled water, or deionized water. Doing so will cause damage to the pH probe.
- 10.2 Never use your finger to touch the glass membrane or use other material to rub it. Doing so could generate static electricity and cause measurement errors.
- 10.3 Avoid testing in high (>113°F) or low (<41°F) temperature solutions as it will cause greater measurement error and potential damage to the probe. Test your samples and perform calibration close to room temperature as much as possible.
- 10.4 Never test oily liquids.
- 10.5 Make sure the battery cap is completely closed with the red O-ring. Otherwise, the waterproof rating could be compromised.




# 11 Troubleshooting Guide

Trouble	Reason	How to fix
<p>Cannot calibrate</p>	Incorrect calibration order	Power on the tester, calibrate pH7 first, then pH4. After pH4 is calibrated, if you want to calibrate pH7 again, you need to reboot the tester.
	Poor quality standard solutions	Replace with fresh and clean standard calibration solutions made by legitimate manufacturers.
	Contaminated probe	Clean the probe with Apera's cleaning solution or detergent water.
	Aged probe	Replace the probe.
	Dried-out probe	Soak the probe in the 3M KCL soaking solution for at least 1 hour.
	Probe is not fully submerged in the solution	Make sure the probe is fully immersed in the solution at least 1 inch deep.
	Air bubbles around the sensor	Make a quick stir in the solution to remove air bubbles.
<p>Reading is always slowly changing, won't stabilize.</p>	Contaminated probe	Clean the probe with Apera's cleaning solution or detergent water.
	Clogged junction	Clean the probe with Apera's cleaning solution, then soak in 3M KCL soaking solution overnight.
	Aged probe	Replace the probe.
<p>Display similar readings in any solutions or always display 7.0 pH</p>	Testing pH of low ionic strength solutions like tap water, drinking water, RO water, distilled water	Be patient, wait for 1-5 minutes to reach a fully stabilized reading. If still not stabilizing, add 3M KCL soaking solution to your test water at 1:1000 ratio(e.g. 1ml to 1000ml or 1 teaspoon to 1 gallon)
	Broken probe	If you don't find any visible damage of the probe and it's within the 1-year probe warranty, contact your point of purchase for warranty fulfillment; if there is visible damage or the probe is aged, replace the probe.
<p>Reading keeps jumping</p>	Probe is not fully submerged in the solution	Make sure the probe is fully immersed in the solution at least 1 inch deep.
	Air bubbles around the sensor	Make a quick stir in the solution to remove air bubbles.
	Probe is not properly connected or the pin connector is broken.	Check the probe's connector, make sure it's not broken and is connected. Align the probe and instrument correctly before plugging in. Never force it. Ensure that the probe connector is not exposed in the air too long.
<p>Calibration is successful, but reading is not accurate</p>	Aged probe	Replace the probe.
	Air bubbles around the sensor	Make a quick stir in the solution to remove air bubbles.
	Clogged junction	Clean the probe with cleaning solution, the soak it in 3M KCL soaking solution overnight
	Comparison with other testers, test strips, or drop tests	To compare with other testers, make sure to calibration at the same pH7 standard, the test pH4. Whichever gives more accurate reading is the more accurate one. Test strips or drop tests' accuracy is not comparable to pH meters'.





Out of range reminder for pH



Out of range reminder for temperature

12 Technical Specs

Range	0.0-14.0 pH 0-50°C (32-122 °F)
Resolution	0.1 pH, 0.1°C /0.1 °F
Accuracy	±0.1 pH, ±0.1°C /±0.1 °F
Temperature compensation	Automatic
Calibration	Automatic 1 to 3 points (7/4/10) *pH 10.01 solution sold separately
Unit	pH, °C, °F
Power supply	4-AAA alkaline batteries
Backlight	White (measurement) ; Green (calibration) ; Red (errors)
Reading hold	Manual
Warranty	Two years for the instrument, one year for the probe
pH probe	Low-resistance lithium glass membrane, double-junction, blue gel electrolyte
Successful calibration indicators	M (7.00 pH), L(4.00 pH), H(10.01 pH)
Low battery reminder	
Waterproof rating	IP67
Reading stabilization icon	

What's in the box



13 Accessories

**pH Calibration Kit  
(pH 4/7/10, 16oz. each  
& CalPod Solution Organizer)  
SKU: AI1114**



**pH Calibration Kit  
(pH 4/7/10, 16oz. each  
& CalPod Solution Organizer)  
SKU: AI1116**



**Replacement Probes**

**GS1-E  
pH Probe**



**GS2-E  
Soil pH Probe**



**GS5-E  
ORP Probe**



**Probe Care Kit  
SKU: AI1170**

includes 3M KCL soaking solution (4oz.),  
probe cleaning solution (8oz.),  
a CalPod solution organizer, a probe  
cleaning brush, and pH 4/7/10 solutions



### How Long Does the Coverage Last?

Apera Instruments® (Apera) warrants the GroStar® GS1 pH Pen Tester (Product) for a period of 24 months for the instrument and 12 months for the probe from date of purchase by original purchaser or consumer. Proof of purchase is required for the warranty to be effective (store sales receipt for Product showing model number, payment and date of purchase). This warranty is non-transferable and terminates if the original purchaser/consumer sells or transfers the Product to a third party.

### What is Covered?

Apera warrants the Product against defects in material and workmanship when used in a normal manner, in accordance with Apera instruction manuals. If Apera is provided with valid proof of purchase (as defined above) and determines the Product is defective, Apera may, in its sole discretion either (a) repair the Product with new or refurbished parts, or (b) replace the Product with a new or refurbished Product.

### What is NOT Covered?

This warranty does not apply to equipment, component or part that was not manufactured or sold by Apera, and shall be void if any such item is installed on a Product. Further, this warranty does not apply to replacement of items subject to normal use, wear and tear and expressly excludes:

- Cosmetic damage such as stains, scratches and dents
- Damage due to accident, improper use, negligence, careless operation or handling of Product not in accordance with Apera instruction manuals, or failure to maintain or care for Product as recommended by Apera
- Damage caused by use of parts not assembled/installed as per Apera instructions
- Damage caused by use of parts or accessories not produced or recommended by Apera
- Damage due to transportation or shipment of Product
- Product repaired or altered by parties other than Apera or its authorized agents
- Product with defaced, missing or illegible serial numbers
- Products not purchased from Apera or an Apera-authorized distributor or reseller.

### Limitation of Liability & Acknowledgments

TO THE MAXIMUM EXTENT PERMITTED BY LAW, THIS WARRANTY AND THE REMEDIES SET OUT ABOVE ARE EXCLUSIVE AND IN LIEU OF ALL OTHER WARRANTIES, GUARANTEES AND REMEDIES (ORAL OR WRITTEN, EXPRESS OR IMPLIED). EXCEPT AS PROVIDED IN THIS WARRANTY AND TO THE MAXIMUM EXTENT PERMITTED BY LAW, APERA INSTRUMENTS IS NOT RESPONSIBLE FOR SPECIAL, INCIDENTAL OR CONSEQUENTIAL LOSS OR DAMAGES, OR ANY OTHER LOSS OR DAMAGES RESULTING FROM SALE OR USE OF THE PRODUCT, OR BREACH OF WARRANTY, HOWEVER CAUSED, INCLUDING DAMAGES FOR LOST PROFITS, PERSONAL INJURY OR PROPERTY DAMAGE.

IT IS UNDERSTOOD AND AGREED BY CONSUMER UPON PURCHASE OF A PRODUCT THAT, EXCEPT AS STATED IN THIS WARRANTY, APERA INSTRUMENTS IS NOT MAKING AND HAS NOT MADE ANY EXPRESS OR IMPLIED WARRANTY OR OTHER REPRESENTATION REGARDING THE PRODUCT, AND DISCLAIMS ANY WARRANTY OF MERCHANTABILITY OR FITNESS FOR A PARTICULAR PURPOSE TO THE EXTENT PERMITTED BY LAW. ANY WARRANTIES WHICH ARE IMPOSED BY LAW AND CANNOT BE DISCLAIMED ARE HEREBY LIMITED IN DURATION TO THE PERIOD AND REMEDIES PROVIDED IN THIS WARRANTY.

SOME JURISDICTIONS (STATES OR COUNTRIES) DO NOT ALLOW EXCLUSION OR LIMITATION FOR INCIDENTAL OR CONSEQUENTIAL DAMAGES, OR LIMITATION ON HOW LONG AN IMPLIED WARRANTY LASTS, SO THE ABOVE LIMITATION OR EXCLUSION MAY NOT BE APPLICABLE. IF ANY PROVISION OF THIS WARRANTY IS JUDGED TO BE ILLEGAL, INVALID OR UNENFORCEABLE, THE REMAINING PROVISIONS OF THE WARRANTY SHALL REMAIN IN FULL FORCE AND EFFECT.

### Governing Law; Authority

This warranty is governed by the laws of the state of country where Product is purchased, without regard to its choice of law principles. Except as allowed by law, Apera does not limit or exclude other rights a consumer may have with regard to the Product. No Apera distributor, employee or agent is authorized to modify, extend or otherwise change the terms of this warranty.



Address: 6656 Busch Blvd, Columbus Ohio 43229

Tel: 1-614-285-3080

Email: [info@aperainst.com](mailto:info@aperainst.com)

Website: [aperainst.com](http://aperainst.com)